


alternative calibration with
adjust ring
(not included in delivery)

order number: 0641-32

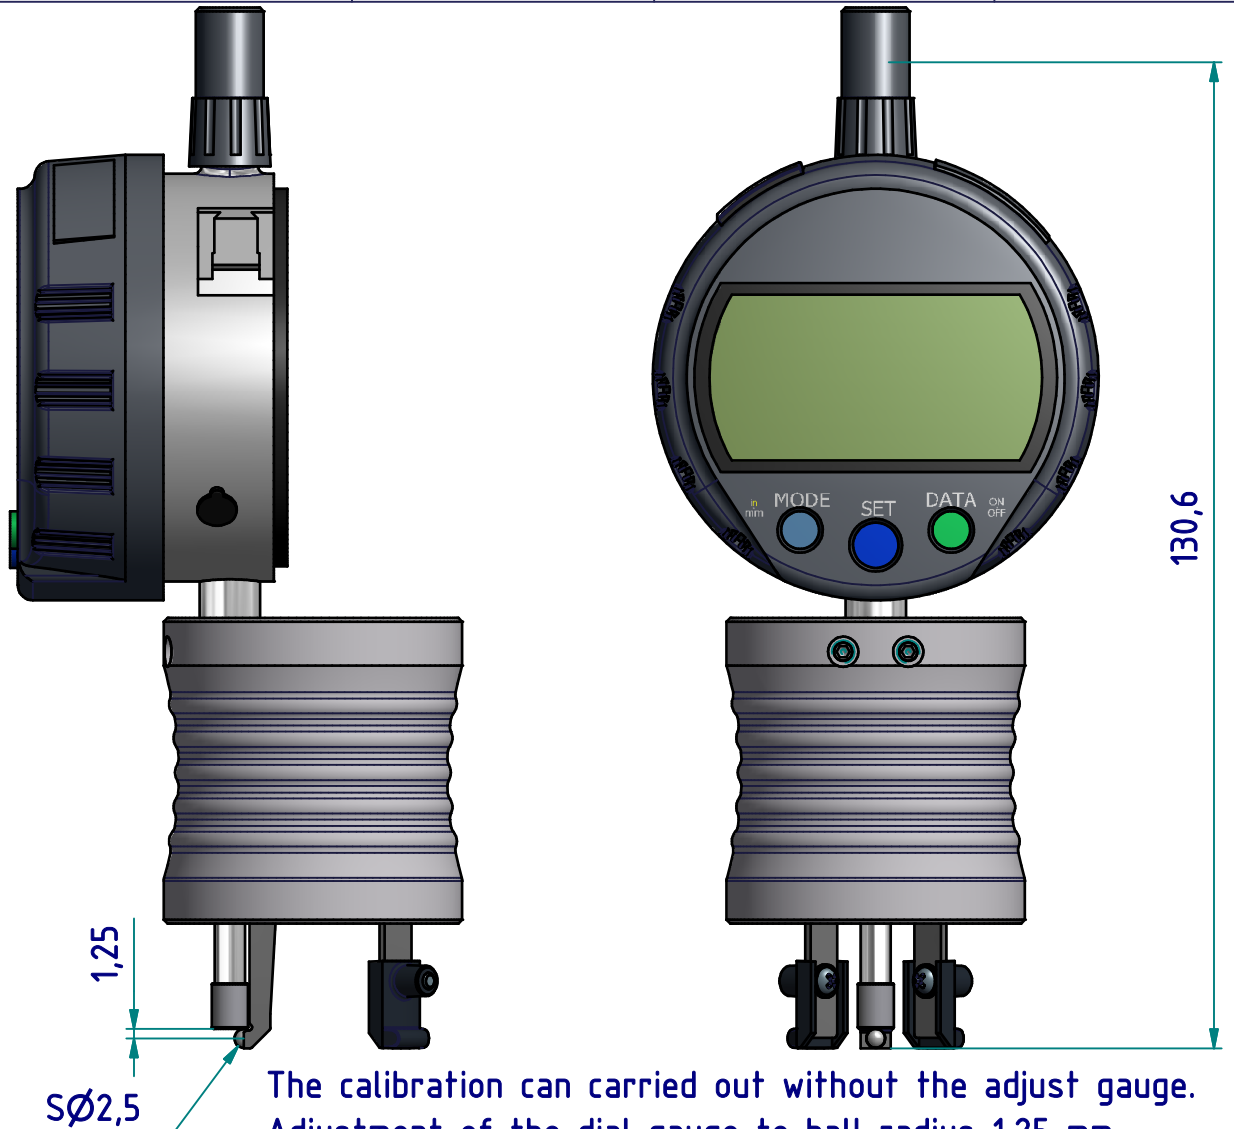

The calibration can be carried out without the adjust gauge.
Adjustment of the dial gauge to ball radius 1,25 mm,

subject to technical alterations

<p>type: aerosol</p> <p>range: 4,6 - 5,4 mm</p> <p>range of indication: 1,25 - 10,3 mm</p> <p>digital step: 0,01 mm</p> <p>scale interval:</p> <p>measuring force: 0,7 - 1,3 N</p> <p>weight: ca. 280 g</p>	<p>acceptable deviations VDI/VDE/DGQ 2618 Bl. 12.1/13.1)</p> <p>max. permissible errors "G": 0,02 mm</p> <p>repeatability "r": 0,02 mm</p> <p>reference temperature: 20° C</p> <p>operation temperature: 10° C - 30° C</p> <p>storage temperature: -10° C - 50° C</p>	<p>scale: 1:1</p> <p>drawing-nr.: IDW-AE2105-DB_e</p> <p>revision status: 2090</p> <p>revision date: 19.09.2014/MHe</p>
--	--	---

4

3

2

1

AE2105

calibration with
adjust gauge



measurement

D

C

B

A

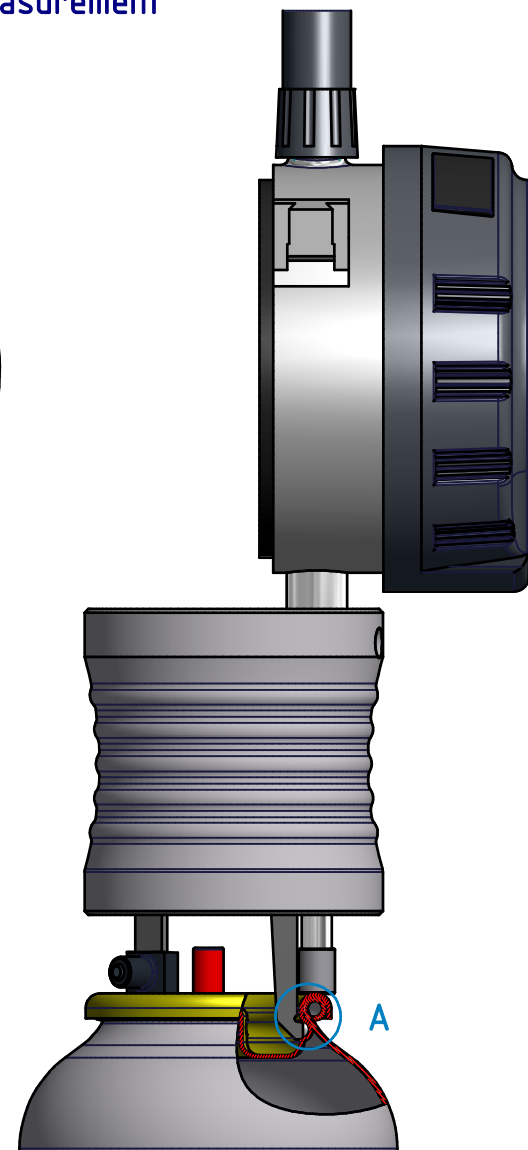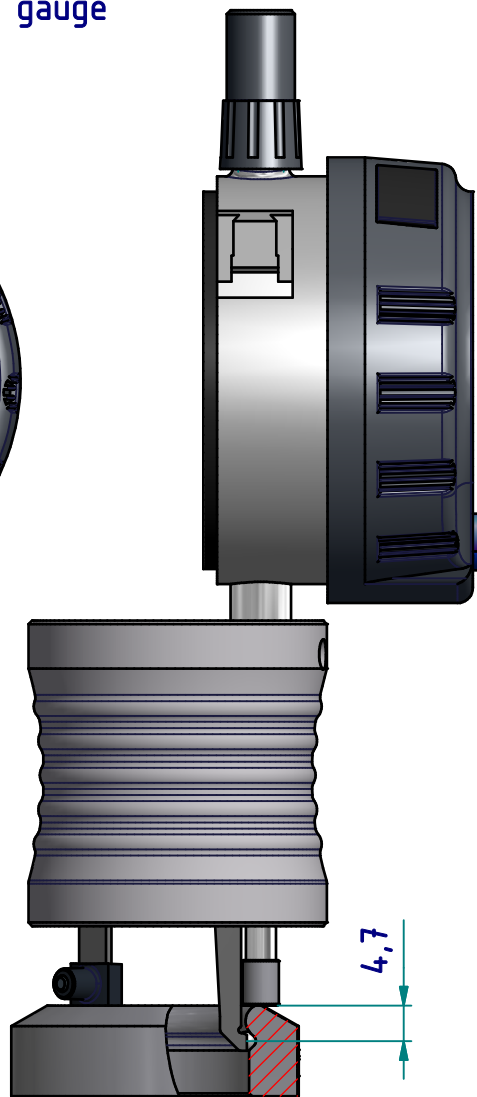

A (2:1)

